

PHONG KHAM DA KHOA MEDIC NHA TRANG

MONTHLY HAEMATOLOGY

CYCLE 10 SAMPLE 11

Explanation of codes used in this report

R - Results removed due to reconstitution error
N - No result returned
C - Result corrected

Authorised by: Stephen Doherty, RIQAS Manager

Issue No: 1

Issue Date: 20/11/2017

BỘ Y TẾ
ĐẠI HỌC Y DƯỢC THÀNH PHỐ HỒ CHÍ MINH
TRUNG TÂM KIỂM CHUẨN CHẤT LƯỢNG XÉT NGHIỆM Y HỌC
Địa chỉ: số 131 Nguyễn Chí Thanh, Phường 9, Quận 5, TPHCM.
Email1: TRUNGTAMKIEMCHUAN@GMAIL.COM
Email2: EQA.QCC.UMP@GMAIL.COM
Website: WWW.QCCUMP.COM
Điện thoại: 08.38531058 - Fax: 08.38531049




Haemoglobin, g/dl





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	5503	14.437	2.1	0.01	0.38	505
ABX Micros/Minos/ABC VET	170	14.292	2.6	0.04	0.37	18

▲ Your Result	14.700	SDI	1.09
		RMSDI	Too Few
■ Mean for Comparison	14.292	TS	68
		RMTS	Too Few
		%DEV	2.9
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	4.19%
Acceptable limits of performance for RIQAS	4.30%

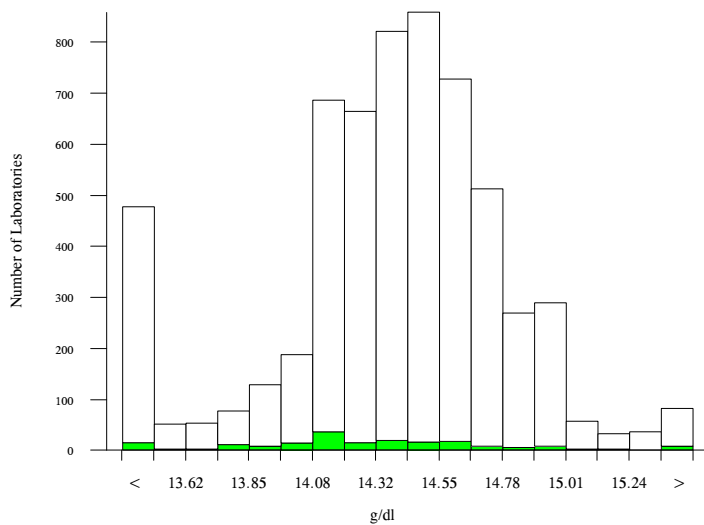

Method	N	Mean	CV%	U _m
Sysmex XN Series	622	14.553	1.1	0.01
Sysmex XT series	468	14.420	1.0	0.01
Sysmex XS series	393	14.469	1.2	0.01
Manual Methods	335	13.168	3.6	0.03
Abbott Cell-Dyn Ruby	294	14.672	1.7	0.02
Siemens/Bayer Advia 120/2120	267	14.496	1.4	0.02
Nihon Kohden Celltac F, Es, Alpha	254	14.577	1.9	0.02
Sysmex KX 21	232	14.343	1.7	0.02
Mindray BC 2000/3000 series	216	14.477	2.7	0.03
ABX Micros/Minos/ABC VET	170	14.292	2.6	0.04
Beckman Coulter LH700 Series	175	14.449	1.2	0.02
Beckman Coulter DxH Series	161	14.194	1.0	0.01
ABX Pentra	134	14.414	1.4	0.02
Sysmex XP Series	129	14.264	1.7	0.03
Mindray BC-6600/6800	107	14.353	0.9	0.01
Beckman Coulter Ac. T 5 series	105	14.428	1.2	0.02
ABX Pentra 60/80 /Yumizen H500	103	14.411	1.3	0.02
Sysmex XE-2100	95	14.486	1.1	0.02
Mindray BC 5000/5150	80	14.360	1.6	0.03
Mindray BC 5100/5180/5300/5380	76	14.365	1.6	0.03
Medonic M series/Swelab	71	14.540	2.3	0.05

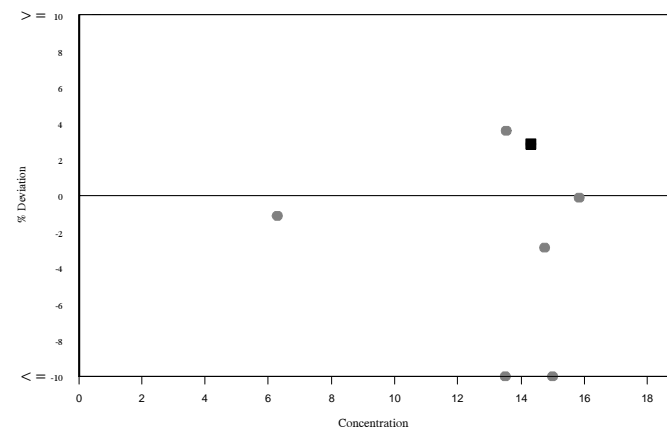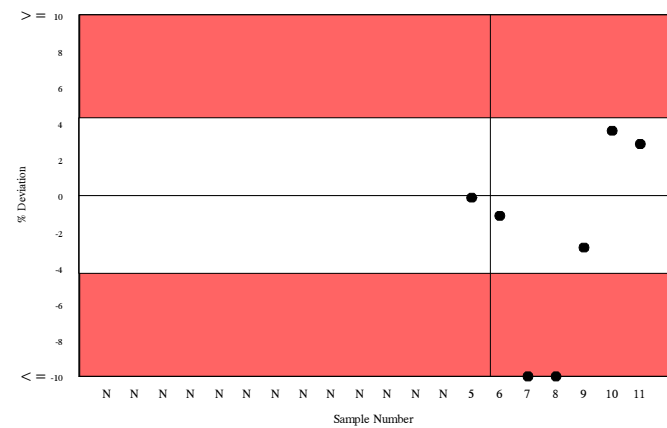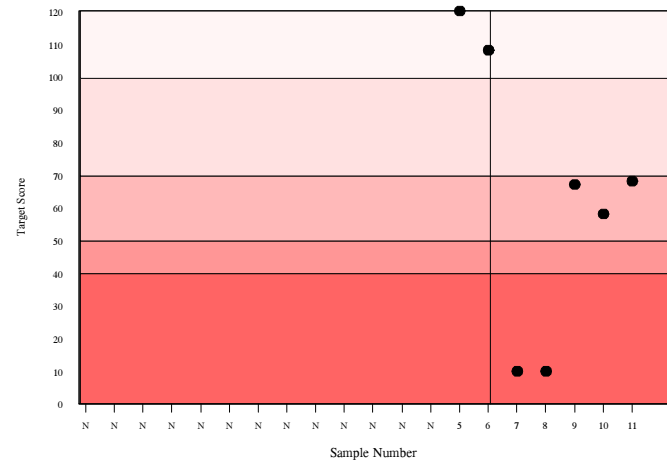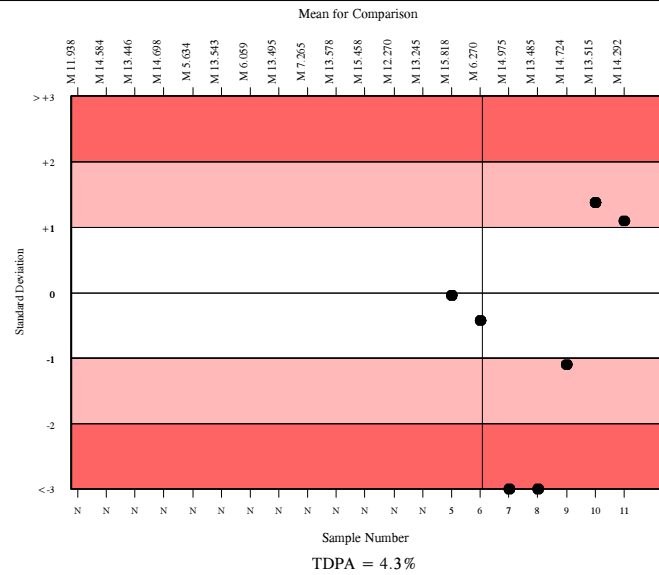

RIQAS




Haematocrit (HCT), %





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	5654	43.180	5.8	0.04	1.60	348
ABX Micros/Minos/ABC VET	168	42.908	3.2	0.13	1.59	20

▲ Your Result	43.900	SDI	0.62
		RMSDI	Too Few
■ Mean for Comparison	42.908	TS	92
		RMTS	Too Few
		%DEV	2.3
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	3.97%
Acceptable limits of performance for RIQAS	6.10%

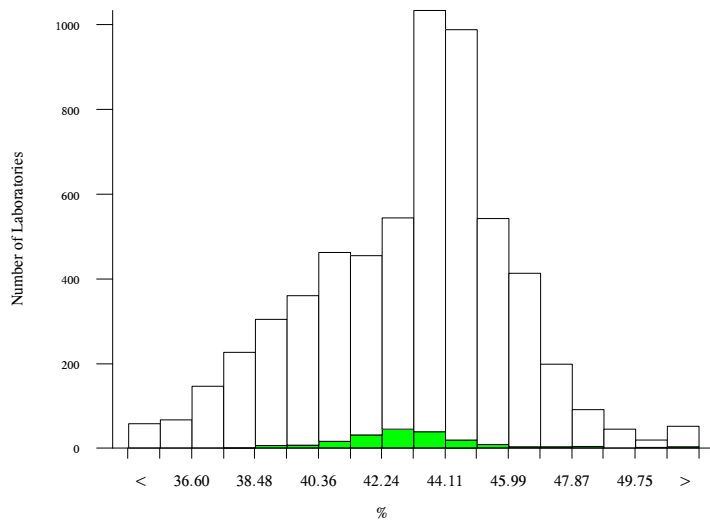

Method	N	Mean	CV%	U _m
Sysmex XN Series	609	44.395	2.1	0.05
Sysmex XT series	475	43.941	2.1	0.05
Sysmex XS series	394	43.976	2.3	0.06
Manual Methods	349	39.899	3.3	0.09
Abbott Cell-Dyn Ruby	287	38.432	2.8	0.08
Siemens/Bayer Advia 120/2120	272	38.123	2.9	0.08
Nihon Kohden Celltac F, Es, Alpha	255	45.078	3.4	0.12
Sysmex KX 21	227	41.817	3.0	0.11
Mindray BC 2000/3000 series	210	45.305	3.2	0.13
ABX Micros/Minos/ABC VET	168	42.908	3.2	0.13
Beckman Coulter LH700 Series	169	44.444	1.7	0.07
Beckman Coulter DxH Series	170	44.362	1.9	0.08
Sysmex XP Series	127	41.496	2.4	0.11
ABX Pentra	128	41.172	1.9	0.09
Mindray BC-6600/6800	110	46.817	1.9	0.10
Beckman Coulter Ac. T 5 series	100	40.826	2.1	0.11
ABX Pentra 60/80 /Yumizen H500	97	41.014	1.7	0.09
Sysmex XE-2100	96	44.238	1.9	0.11
Mindray BC 5000/5150	81	46.117	3.3	0.21
Mindray BC 5100/5180/5300/5380	73	47.055	2.9	0.20
Medonic M series/Swelab	72	43.065	2.8	0.18

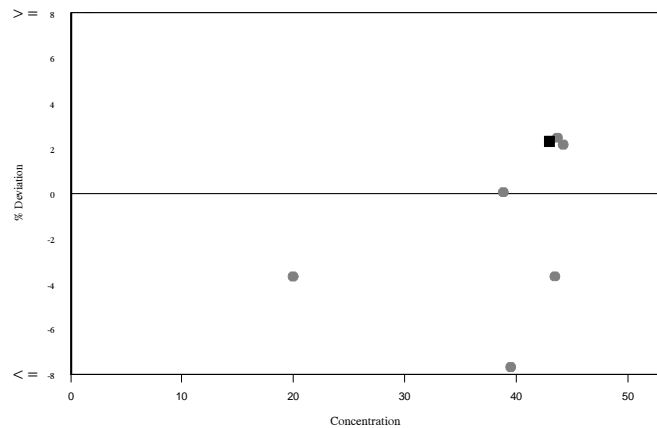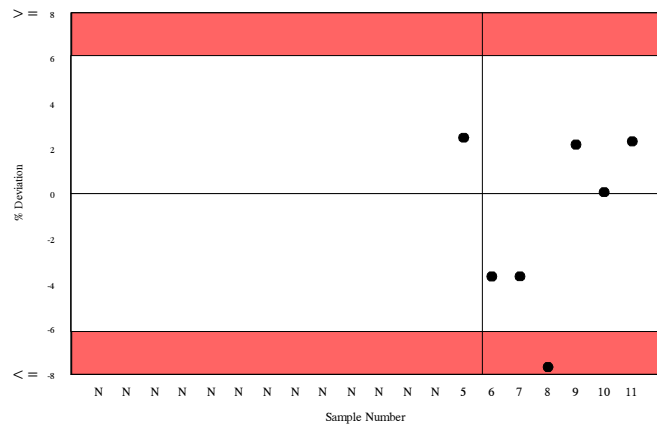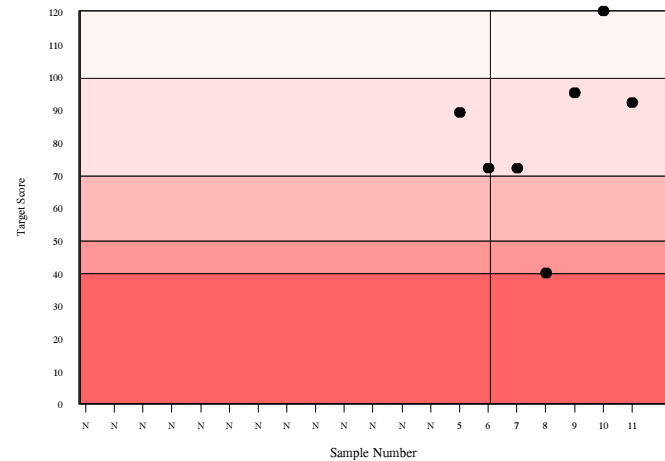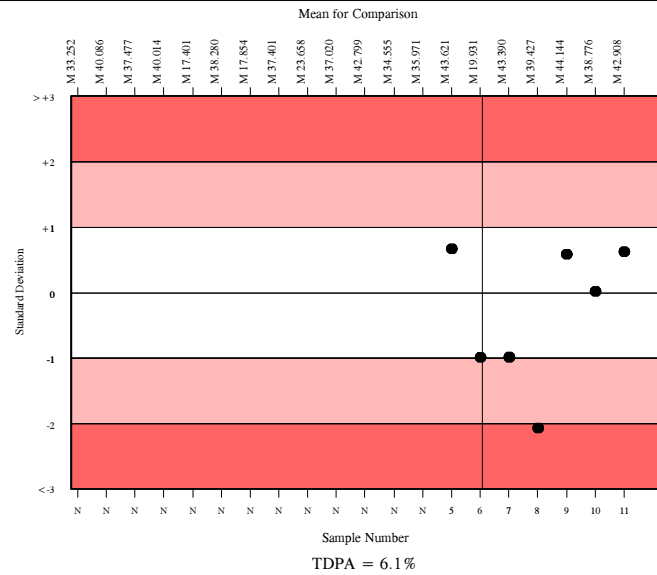


RIQAS

MCH, pg





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	5138	28.511	2.3	0.01	0.89	426
ABX Micros/Minos/ABC VET	164	28.453	3.1	0.09	0.89	20

▲ Your Result	28.600	SDI	0.17
		RMSDI	Too Few
■ Mean for Comparison	28.453	TS	120
		RMTS	Too Few
		%DEV	0.5
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	2.5%
Acceptable limits of performance for RIQAS	6.10%

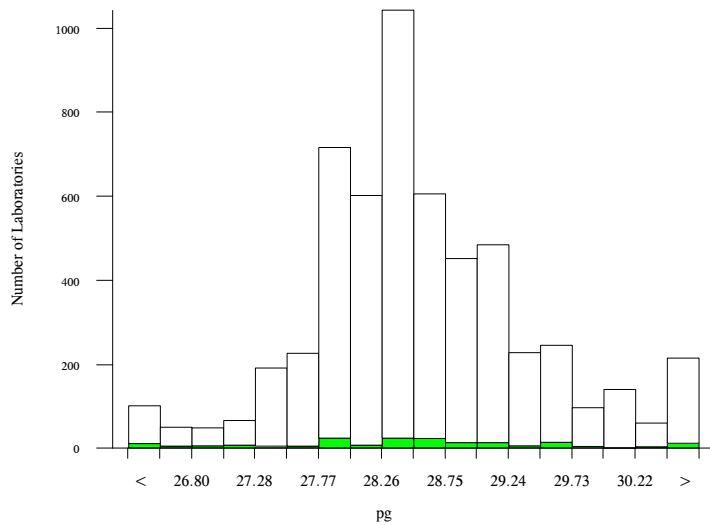

Method	N	Mean	CV%	U _m
Sysmex XN Series	618	28.226	1.3	0.02
Sysmex XT series	479	28.258	1.5	0.02
Sysmex XS series	394	28.546	1.3	0.02
Abbott Cell-Dyn Ruby	292	29.121	2.6	0.05
Siemens/Bayer Advia 120/2120	273	29.466	2.0	0.05
Nihon Kohden Celltac F, Es, Alpha	256	28.852	2.4	0.05
Sysmex KX 21	227	28.499	2.1	0.05
Mindray BC 2000/3000 series	217	28.471	3.0	0.07
Beckman Coulter DxH Series	169	28.083	1.6	0.04
Beckman Coulter LH700 Series	171	28.188	1.3	0.04
ABX Micros/Minos/ABC VET	164	28.453	3.1	0.09
ABX Pentra	134	28.310	1.7	0.05
Sysmex XP Series	131	28.606	2.1	0.07
Mindray BC-6600/6800	109	28.594	1.4	0.05
Beckman Coulter Ac. T 5 series	106	28.379	1.3	0.05
ABX Pentra 60/80 /Yumizen H500	100	28.435	1.2	0.04
Sysmex XE-2100	96	28.321	1.3	0.05
Mindray BC 5000/5150	79	28.517	1.7	0.07
Mindray BC 5100/5180/5300/5380	74	28.663	1.5	0.06
Medonic M series/Swelab	69	28.930	1.8	0.08
Sysmex XN-L Series (350/450/550)	64	28.170	1.1	0.05

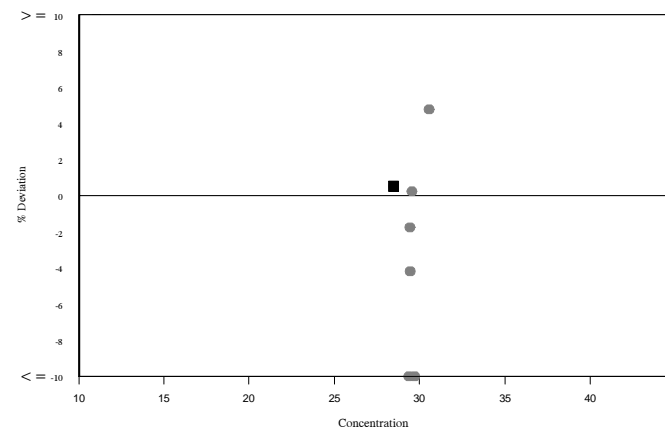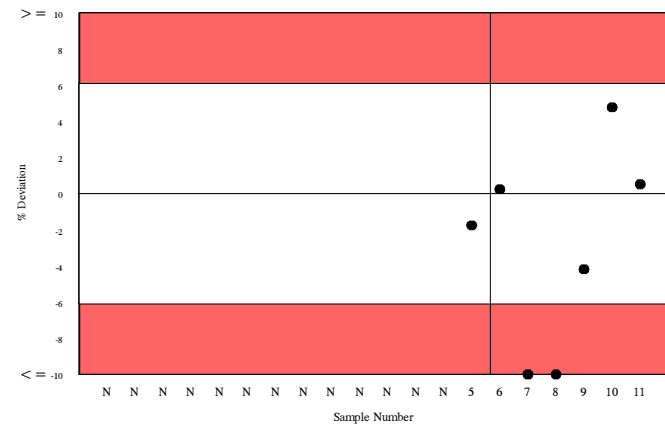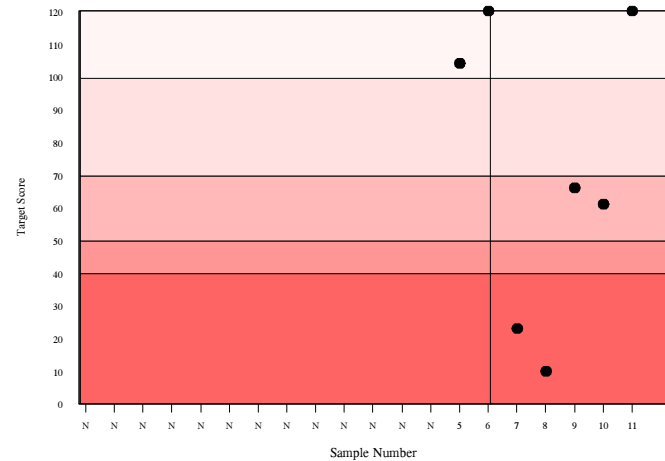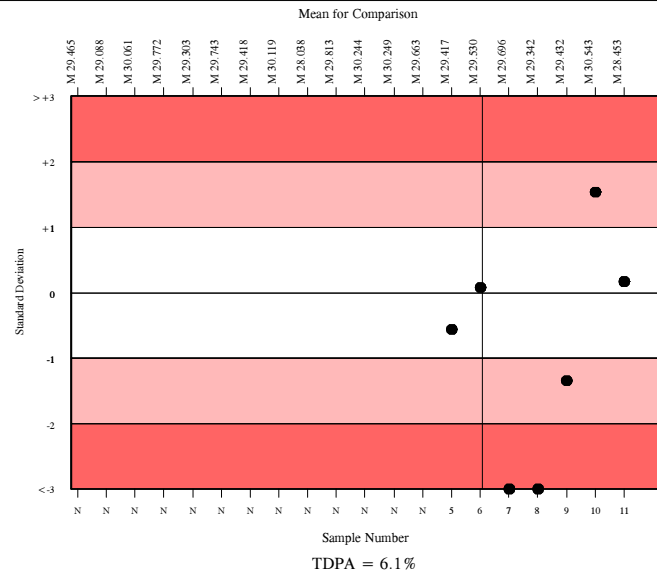


RIQAS

MCHC, g/dl





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	5086	33.088	5.3	0.03	1.23	467
ABX Micros/Minos/ABC VET	167	33.172	3.5	0.11	1.23	15

▲ Your Result	33.500	SDI	0.27
		RMSDI	Too Few
■ Mean for Comparison	33.172	TS	120
		RMTS	Too Few
		%DEV	1.0
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	1.27%
Acceptable limits of performance for RIQAS	6.10%

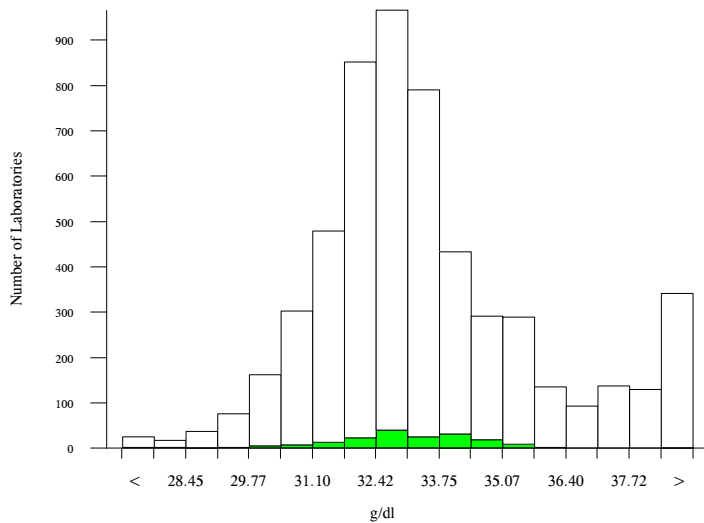

Method	N	Mean	CV%	U _m
Sysmex XN Series	608	32.756	2.0	0.03
Sysmex XT series	465	32.850	2.1	0.04
Sysmex XS series	400	32.870	2.2	0.05
Abbott Cell-Dyn Ruby	284	38.127	2.8	0.08
Siemens/Bayer Advia 120/2120	268	38.037	2.7	0.08
Nihon Kohden Celltac F, Es, Alpha	261	32.307	3.1	0.08
Sysmex KX 21	228	34.314	3.4	0.10
Mindray BC 2000/3000 series	210	31.820	3.2	0.09
Beckman Coulter DxH Series	172	31.948	1.9	0.06
Beckman Coulter LH700 Series	169	32.452	1.9	0.06
ABX Micros/Minos/ABC VET	167	33.172	3.5	0.11
ABX Pentra	129	35.076	2.0	0.08
Sysmex XP Series	128	34.405	2.9	0.11
Mindray BC-6600/6800	110	30.650	1.9	0.07
Beckman Coulter Ac. T 5 series	98	35.373	1.8	0.08
ABX Pentra 60/80 /Yumizen H500	96	35.188	1.9	0.09
Sysmex XE-2100	95	32.649	1.8	0.08
Mindray BC 5000/5150	83	31.104	2.6	0.11
Mindray BC 5100/5180/5300/5380	75	30.479	3.1	0.14
Medonic M series/Swelab	72	33.665	2.4	0.12
Sysmex XN-L Series (350/450/550)	64	32.857	1.6	0.08

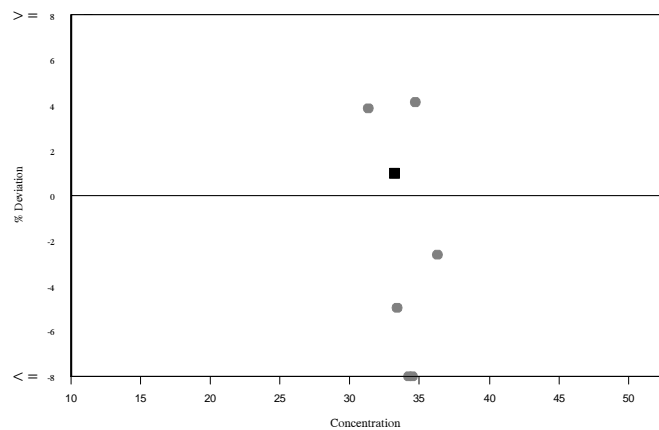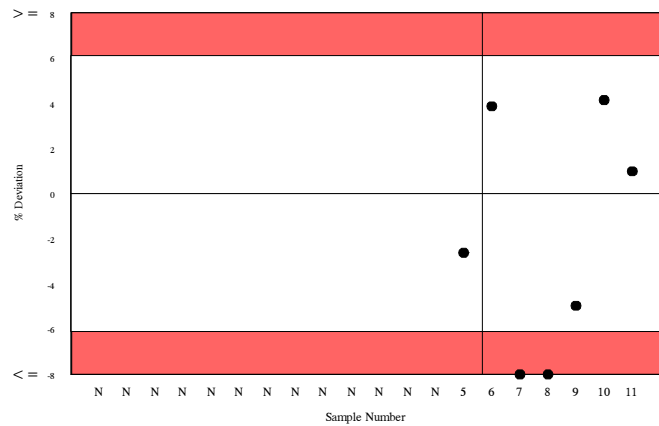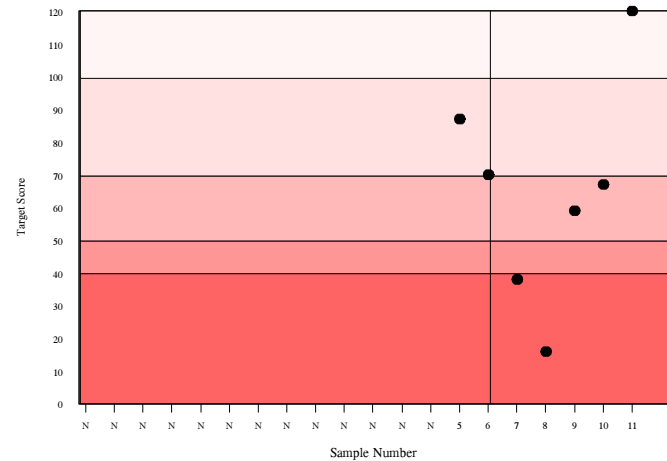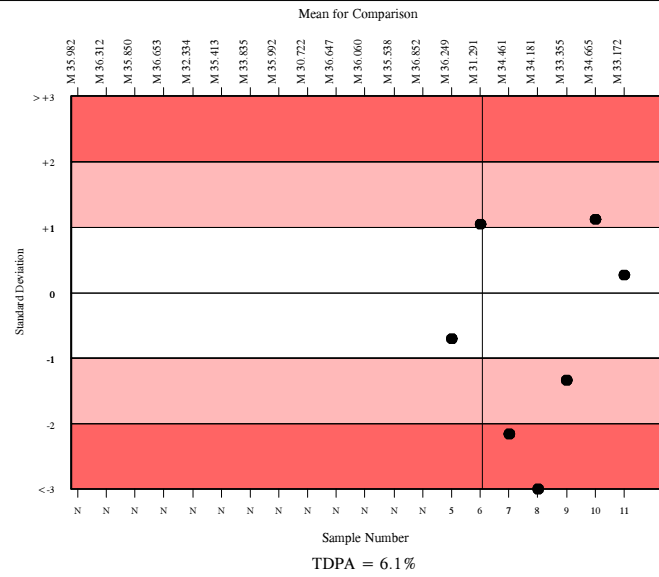






RIQAS

MCV, um3

	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	5215	85.753	5.0	0.07	2.67	352
ABX Micros/Minos/ABC VET	171	85.630	3.0	0.24	2.67	14

▲ Your Result	85.000	SDI	-0.24
		RMSDI	Too Few
■ Mean for Comparison	85.630	TS	120
		RMTS	Too Few
		%DEV	-0.7
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	2.42%
Acceptable limits of performance for RIQAS	6.10%

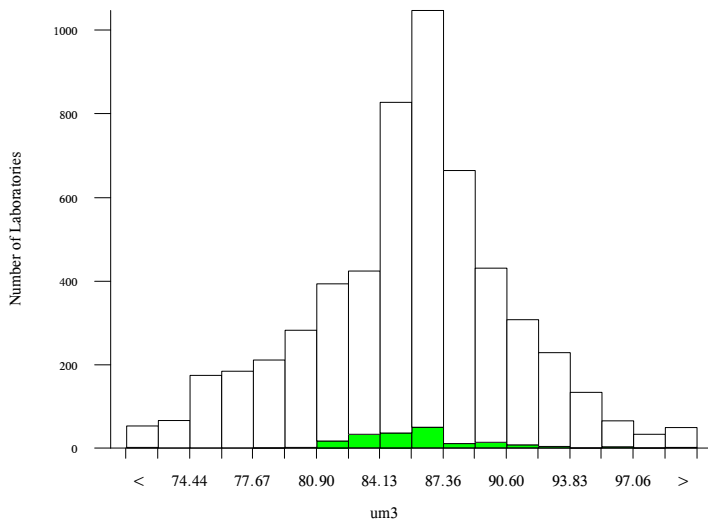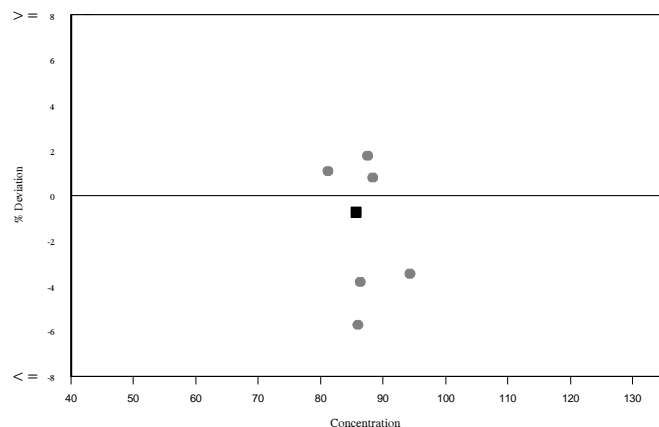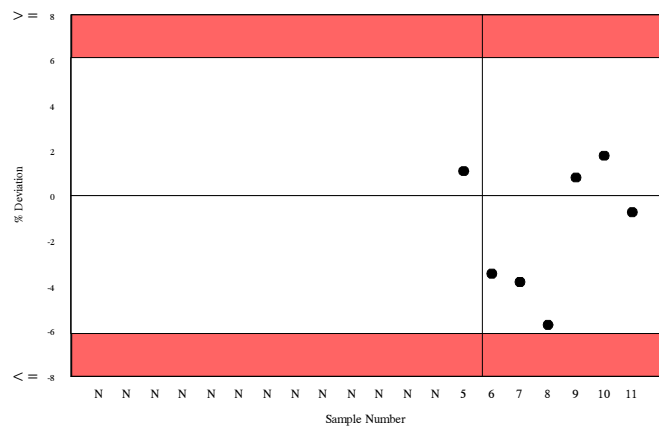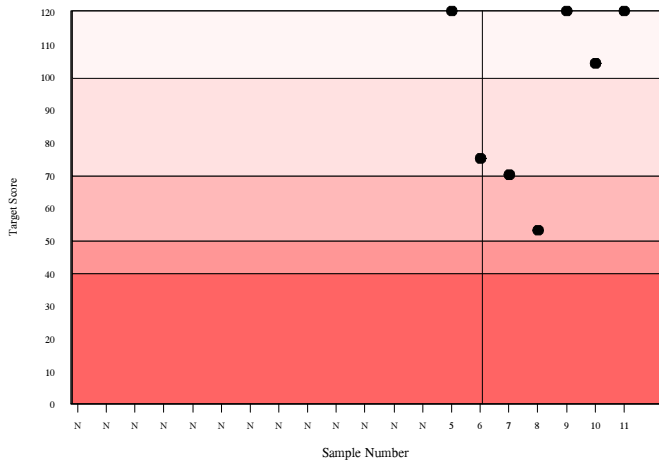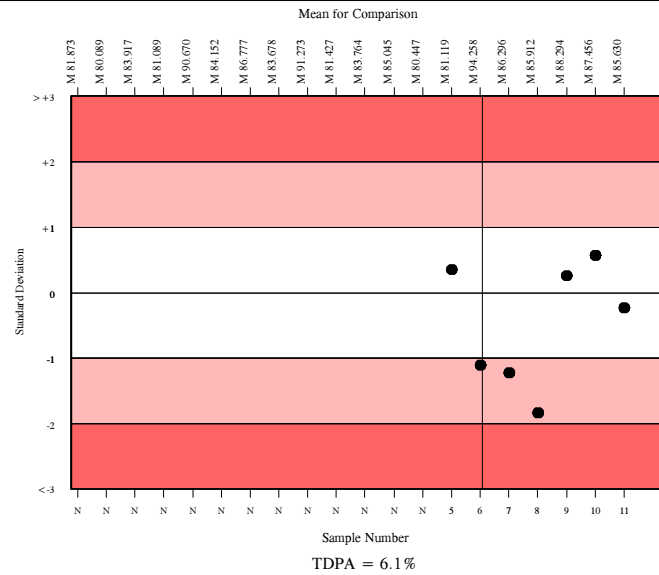


Method	N	Mean	CV%	U _m
Sysmex XN Series	613	86.062	1.7	0.08
Sysmex XT series	466	85.986	1.7	0.08
Sysmex XS series	392	86.837	1.8	0.10
Abbott Cell-Dyn Ruby	293	76.251	2.6	0.15
Siemens/Bayer Advia 120/2120	271	77.410	2.4	0.14
Nihon Kohden Celltac F, Es, Alpha	259	89.402	3.3	0.23
Sysmex KX 21	220	82.779	2.3	0.16
Mindray BC 2000/3000 series	211	89.611	2.9	0.22
Beckman Coulter DxH Series	164	87.525	1.3	0.12
Beckman Coulter LH700 Series	174	86.546	1.8	0.15
ABX Micros/Minos/ABC VET	171	85.630	3.0	0.24
ABX Pentra	131	80.900	1.9	0.17
Sysmex XP Series	132	82.957	2.2	0.20
Mindray BC-6600/6800	108	93.321	1.6	0.18
Beckman Coulter Ac. T 5 series	101	80.247	1.6	0.16
ABX Pentra 60/80 /Yumizen H500	97	80.919	1.4	0.15
Sysmex XE-2100	96	86.476	1.6	0.18
Mindray BC 5000/5150	82	91.745	2.4	0.31
Mindray BC 5100/5180/5300/5380	72	93.979	2.2	0.31
Medonic M series/Swelab	72	85.486	2.5	0.31
Abbott Cell-Dyn 3700	69	90.331	2.1	0.28

Mean Platelet Volume, um3





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	3811	9.652	9.3	0.02	0.66	317
ABX Micros/Minos/ABC VET	121	8.749	5.8	0.06	0.60	9

▲ Your Result	8.600	SDI	-0.25
		RMSDI	Too Few
■ Mean for Comparison	8.749	TS	120
		RMTS	Too Few
		%DEV	-1.7
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	5.8%
Acceptable limits of performance for RIQAS	11.30%

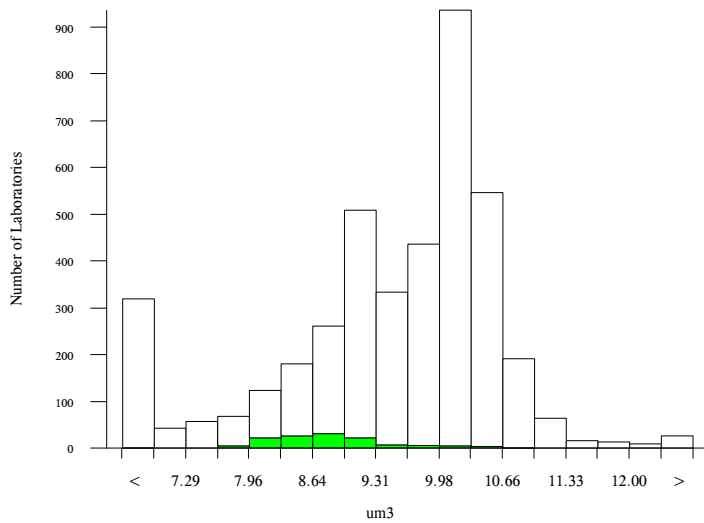

Method	N	Mean	CV%	U _m
Sysmex XN Series	438	10.302	1.9	0.01
Sysmex XT series	332	10.029	2.4	0.02
Sysmex XS series	296	10.423	2.8	0.02
Nihon Kohden Celltac F, Es, Alpha	213	7.639	9.2	0.06
Abbott Cell-Dyn Ruby	213	4.917	9.5	0.04
Siemens/Bayer Advia 120/2120	183	10.344	5.4	0.05
Mindray BC 2000/3000 series	183	9.186	5.8	0.05
Sysmex KX 21	176	9.751	3.5	0.03
Beckman Coulter DxH Series	145	9.149	2.3	0.02
ABX Micros/Minos/ABC VET	121	8.749	5.8	0.06
Beckman Coulter LH700 Series	119	9.119	3.0	0.03
ABX Pentra	96	9.743	3.9	0.05
Sysmex XP Series	91	9.893	3.0	0.04
Mindray BC-6600/6800	88	10.477	2.4	0.03
Sysmex XE-2100	70	10.373	2.3	0.04
Mindray BC 5000/5150	69	9.920	6.7	0.10
ABX Pentra 60/80 /Yumizen H500	63	9.764	3.3	0.05
Beckman Coulter Ac. T 5 series	62	9.734	4.3	0.07
Mindray BC 5100/5180/5300/5380	57	9.136	3.2	0.05
Medonic M series/Swelab	53	8.707	4.8	0.07
Sysmex XN-L Series (350/450/550)	50	10.282	1.8	0.03

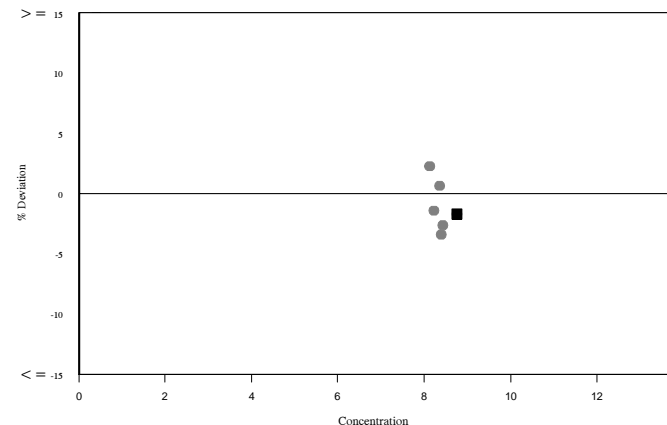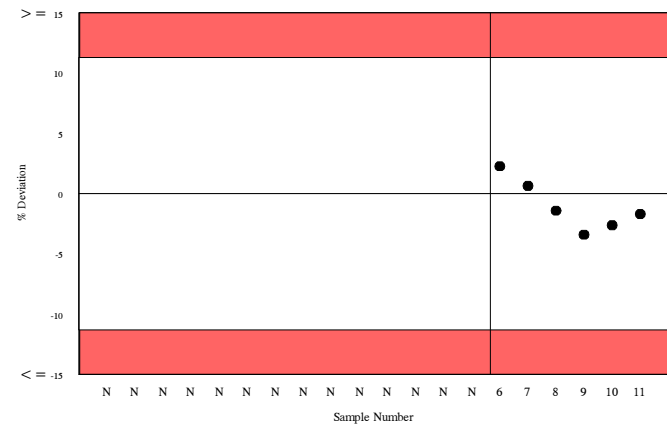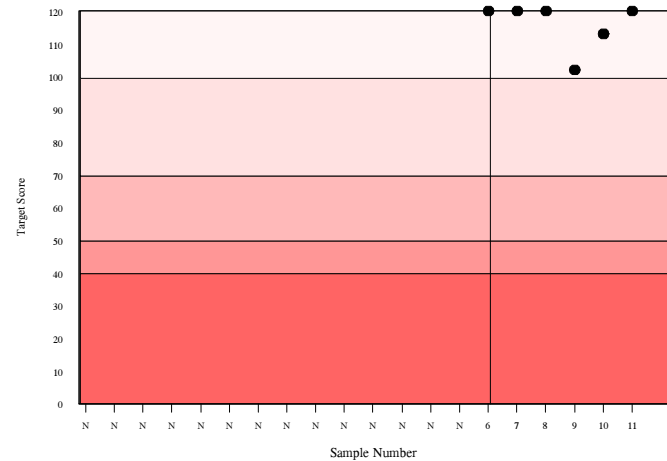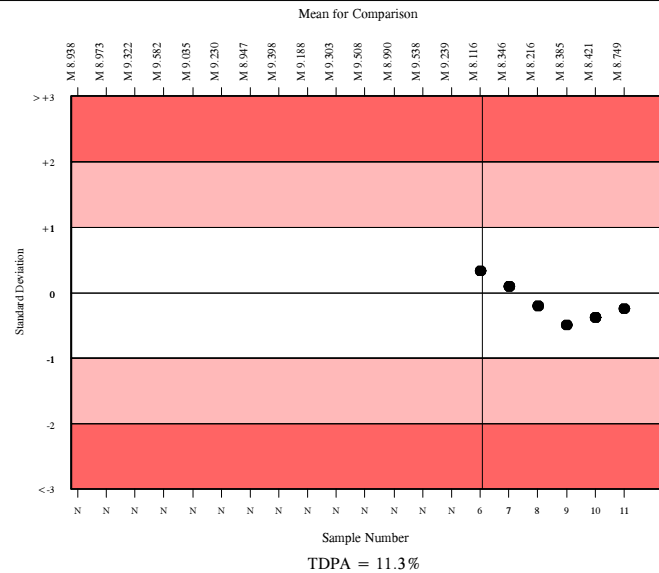






RIQAS

Plateletcrit, %

	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	2013	0.252	12.1	0.00	0.03	196
ABX Micros/Minos/ABC VET	69	0.219	8.6	0.00	0.03	12

▲ Your Result	No Result	SDI	RMSEI	Too Few
▲ Mean for Comparison	0.219	TS	RMTS	Too Few
		%DEV	RM%DEV	Too Few

Acceptable limits derived from Biological Variation	N/A
Acceptable limits of performance for RIQAS	22.50%

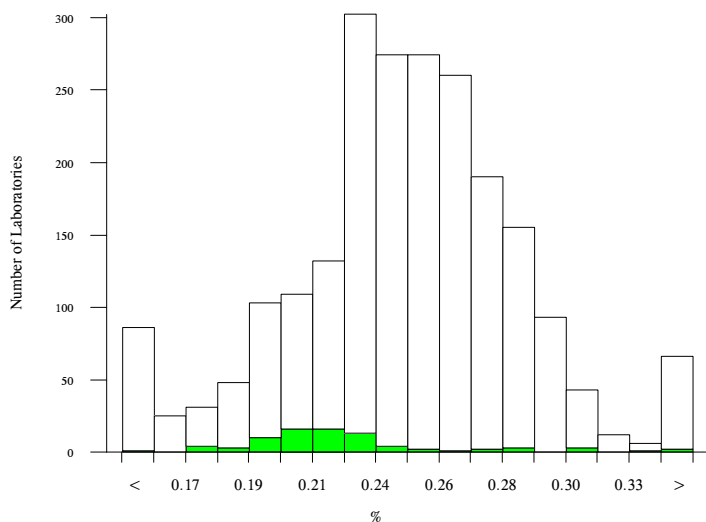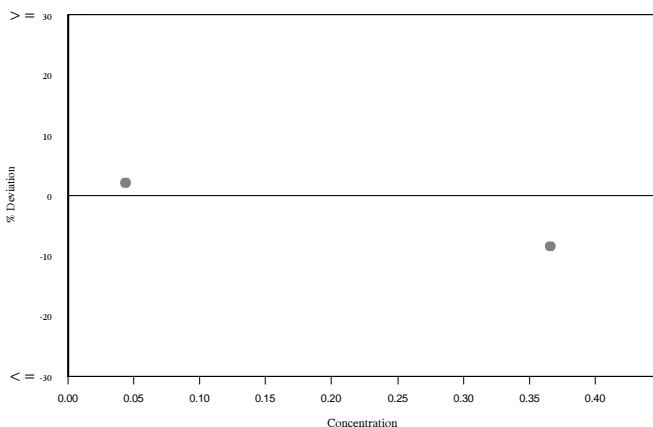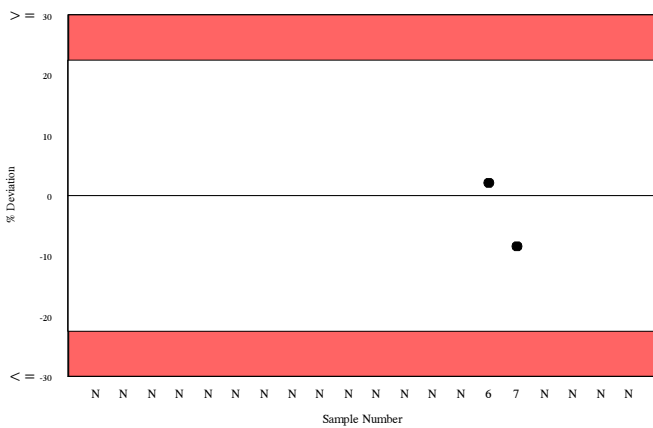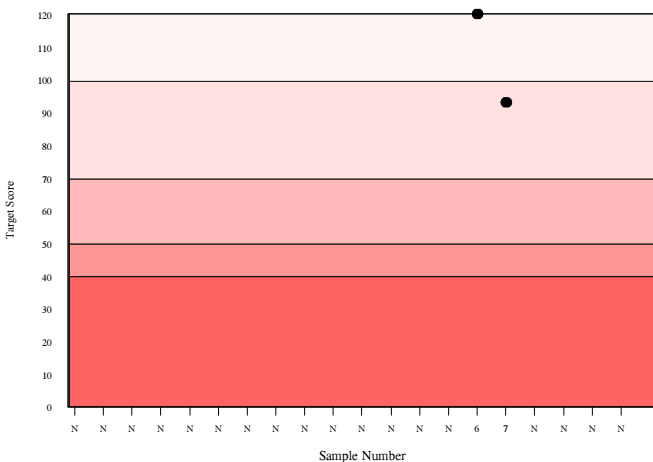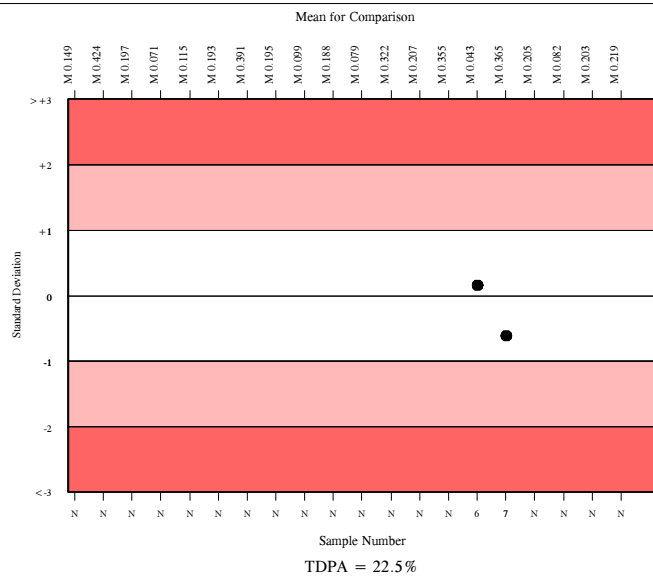

Method	N	Mean	CV%	U _m
Sysmex XN Series	225	0.278	5.3	0.00
Sysmex XT series	219	0.264	6.2	0.00
Nihon Kohden Celltac F, Es. Alpha	179	0.214	11.4	0.00
Mindray BC 2000/3000 series	163	0.239	9.3	0.00
Sysmex XS series	155	0.270	5.6	0.00
Siemens/Bayer Advia 120/2120	83	0.258	8.7	0.00
ABX Micros/Minos/ABC VET	69	0.219	8.6	0.00
Abbott Cell-Dyn Ruby	59	0.166	18.3	0.00
Beckman Coulter LH700 Series	54	0.239	4.8	0.00
Mindray BC 5000/5150	51	0.275	9.3	0.00
Sysmex XP Series	48	0.276	8.3	0.00
Mindray BC 5100/5180/5300/5380	39	0.249	7.9	0.00
ABX Pentra	40	0.265	6.2	0.00
ABX Pentra 120/Nexus series	34	0.261	3.4	0.00
Medonic M series/Swelab	38	0.204	9.6	0.00
ABX Pentra 60/80 /Yumizen H500	34	0.257	6.4	0.00
Beckman Coulter DxH Series	31	0.240	3.9	0.00
Mindray BC-6600/6800	33	0.292	4.7	0.00
Sysmex XE-2100	33	0.244	5.8	0.00
Human Humacount Series	26	0.254	11.9	0.01
Sysmex KX 21	23	0.256	11.7	0.01




RIQAS

Platelets (Impedance Count), x10³/mm³





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	4315	264.105	6.2	0.31	20.23	375
ABX Micros/Minos/ABC VET	160	253.240	6.9	1.73	19.40	21

▲ Your Result	245.000	SDI	-0.42
		RMSDI	Too Few
■ Mean for Comparison	253.240	TS	109
		RMTS	Too Few
		%DEV	-3.3
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	13.4%
Acceptable limits of performance for RIQAS	12.60%

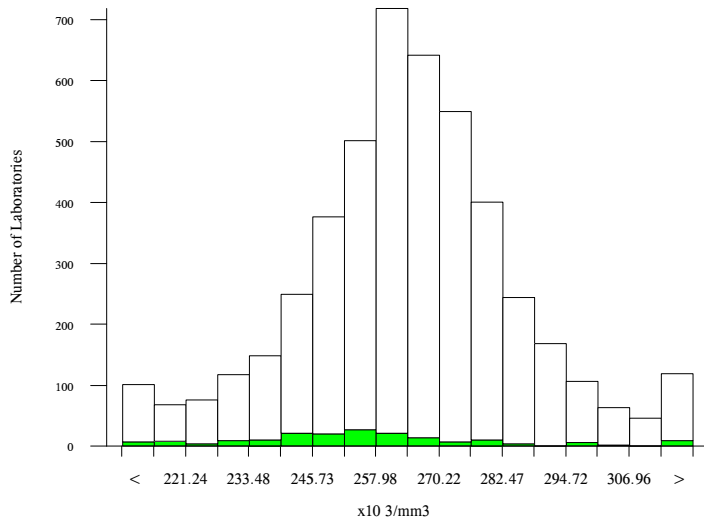

Method	N	Mean	CV%	U _m
Sysmex XN Series	577	267.192	4.0	0.56
Sysmex XT series	413	262.314	3.8	0.62
Sysmex XS series	357	255.590	4.6	0.77
Nihon Kohden Celltac F, Es, Alpha	256	278.014	6.7	1.46
Sysmex KX 21	223	276.808	5.8	1.34
Mindray BC 2000/3000 series	214	262.006	7.3	1.64
ABX Micros/Minos/ABC VET	160	253.240	6.9	1.73
Beckman Coulter LH700 Series	163	262.359	3.9	1.01
Beckman Coulter DxH Series	161	259.002	3.4	0.88
ABX Pentra	126	266.758	4.3	1.27
Sysmex XP Series	128	280.328	5.2	1.62
Mindray BC-6600/6800	107	277.271	3.5	1.17
Beckman Coulter Ac. T 5 series	99	262.747	4.1	1.36
ABX Pentra 60/80 /Yumizen H500	98	265.483	4.2	1.42
Sysmex XE-2100	92	235.424	3.2	1.00
Mindray BC 5000/5150	78	274.359	5.4	2.08
Mindray BC 5100/5180/5300/5380	76	265.935	6.1	2.33
Medonic M series/Swelab	75	232.708	6.4	2.16
Sysmex XN-L Series (350/450/550)	63	267.206	3.8	1.59
Abbott Cell-Dyn 3700	57	272.623	5.4	2.42
Mindray BC 5600/5800	48	274.854	4.2	2.09

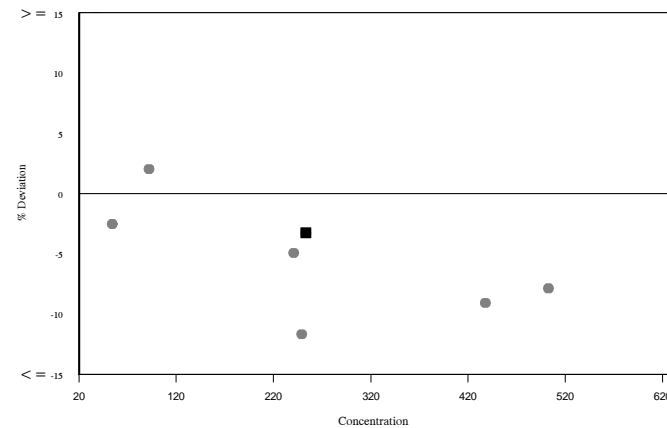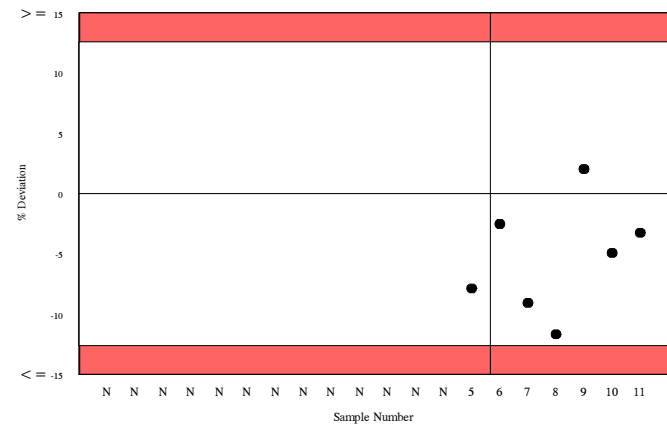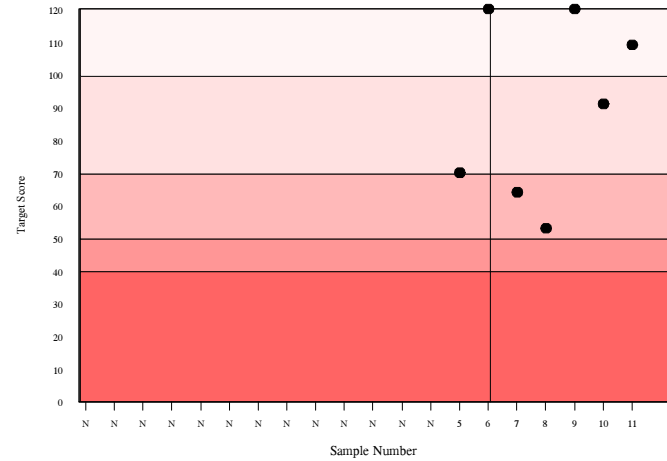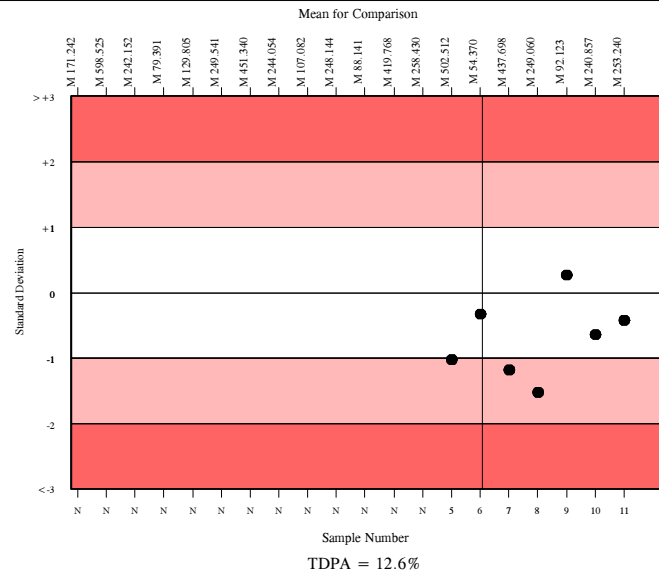


RBC (Impedance Count), x10⁶/mm³





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	4337	5.079	1.9	0.00	0.12	350
ABX Micros/Minos/ABC VET	159	5.036	2.6	0.01	0.12	21

▲ Your Result	5.140	SDI	0.89
		RMSDI	Too Few
■ Mean for Comparison	5.036	TS	77
		RMTS	Too Few
		%DEV	2.1
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	4.4%
Acceptable limits of performance for RIQAS	3.80%

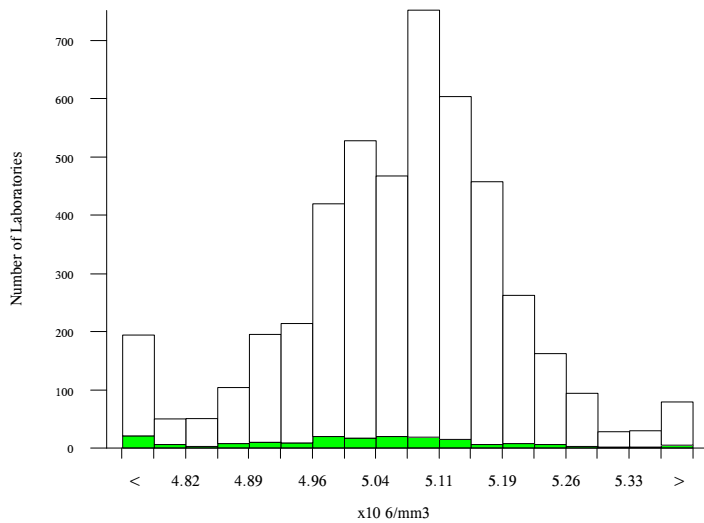

Method	N	Mean	CV%	U _m
Sysmex XN Series	570	5.158	1.3	0.00
Sysmex XT series	420	5.107	1.3	0.00
Sysmex XS series	360	5.073	1.5	0.00
Nihon Kohden Celltac F, Es, Alpha	258	5.050	1.8	0.01
Sysmex KX 21	221	5.047	1.5	0.01
Mindray BC 2000/3000 series	206	5.079	2.3	0.01
ABX Micros/Minos/ABC VET	159	5.036	2.6	0.01
Beckman Coulter LH700 Series	159	5.127	0.9	0.00
Beckman Coulter DxH Series	157	5.054	1.4	0.01
ABX Pentra	127	5.081	1.6	0.01
Sysmex XP Series	125	4.996	1.5	0.01
Mindray BC-6600/6800	103	5.024	1.5	0.01
Beckman Coulter Ac. T 5 series	100	5.090	1.6	0.01
ABX Pentra 60/80 /Yumizen H500	97	5.071	1.6	0.01
Sysmex XE-2100	87	5.122	1.1	0.01
Mindray BC 5000/5150	78	5.025	1.9	0.01
Mindray BC 5100/5180/5300/5380	76	5.017	1.8	0.01
Medonic M series/Swelab	69	5.026	1.9	0.01
Sysmex XN-L Series (350/450/550)	63	5.116	1.0	0.01
Abbott Cell-Dyn 3700	63	5.041	1.6	0.01
Mindray BC 5600/5800	49	5.062	2.1	0.02

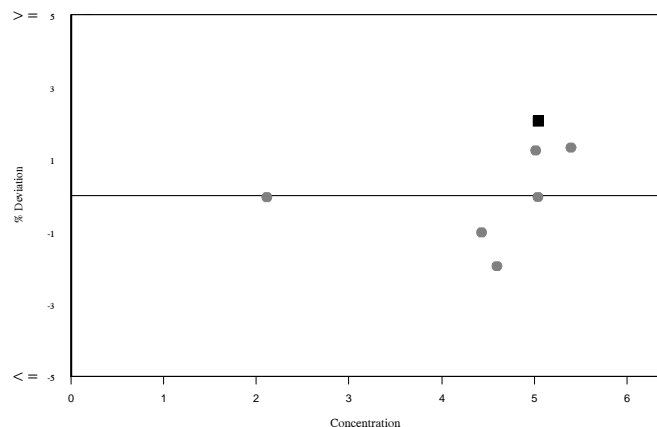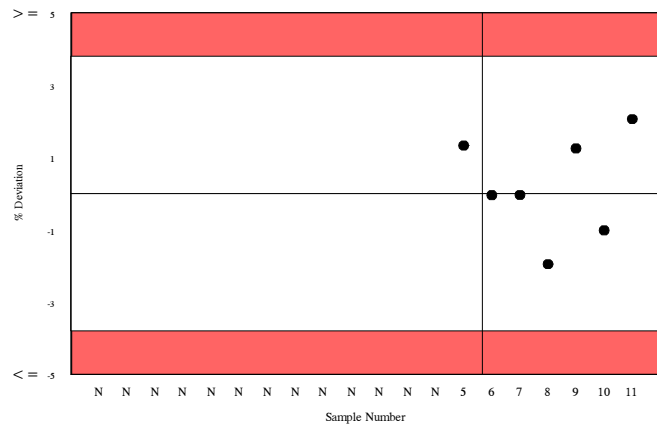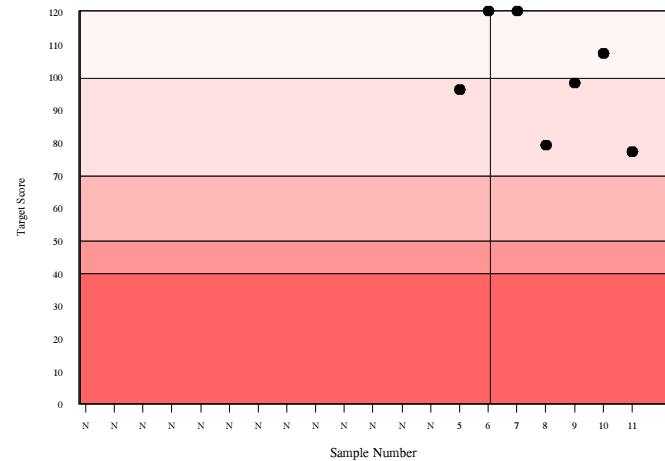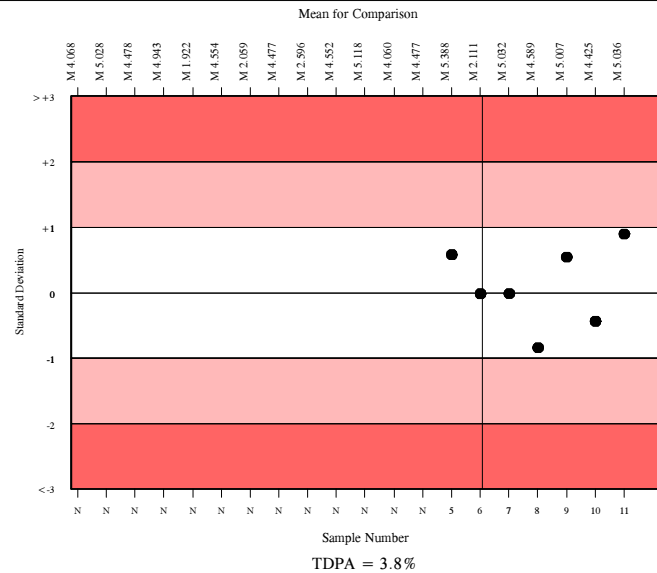


RIQAS

Red Cell Dist. Width CV, %





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	3652	15.382	8.6	0.03	0.89	350
ABX Micros/Minos/ABC VET	78	13.763	8.6	0.17	0.79	9

▲ Your Result	No Result	SDI	Too Few
		RMSDI	
■ Mean for Comparison	13.763	TS	Too Few
		RMTS	
		%DEV	Too Few
		RM%DEV	

Acceptable limits derived from Biological Variation	4.6%
Acceptable limits of performance for RIQAS	9.50%

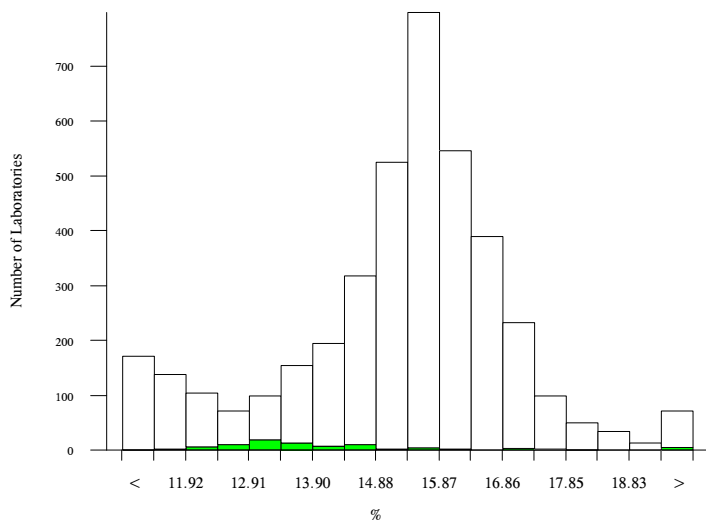

Method	N	Mean	CV%	U _m
Sysmex XN Series	481	15.530	3.5	0.03
Sysmex XT series	350	16.203	3.0	0.03
Sysmex XS series	297	16.438	4.0	0.05
Abbott Cell-Dyn Ruby	194	11.671	4.8	0.05
Nihon Kohden Celltac F. Es. Alpha	192	14.922	5.1	0.07
Siemens/Bayer Advia 120/2120	191	16.613	3.3	0.05
Mindray BC 2000/3000 series	158	14.648	4.5	0.06
Beckman Coulter LH700 Series	138	15.549	1.6	0.03
Sysmex KX 21	129	12.134	6.2	0.08
Beckman Coulter DxH Series	122	15.563	1.7	0.03
ABX Pentra	95	15.053	6.5	0.13
Mindray BC-6600/6800	86	15.707	1.0	0.02
Beckman Coulter Ac. T 5 series	87	14.577	5.8	0.11
ABX Micros/Minos/ABC VET	78	13.763	8.6	0.17
Sysmex XP Series	77	12.075	8.4	0.14
Sysmex XE-2100	76	15.761	2.0	0.05
Mindray BC 5000/5150	66	16.190	7.0	0.17
ABX Pentra 60/80 /Yumizen H500	62	14.301	5.2	0.12
Mindray BC 5100/5180/5300/5380	55	14.569	3.5	0.09
Abbott Cell-Dyn 3700	54	17.089	4.4	0.13
Sysmex XN-L Series (350/450/550)	46	15.532	3.2	0.09

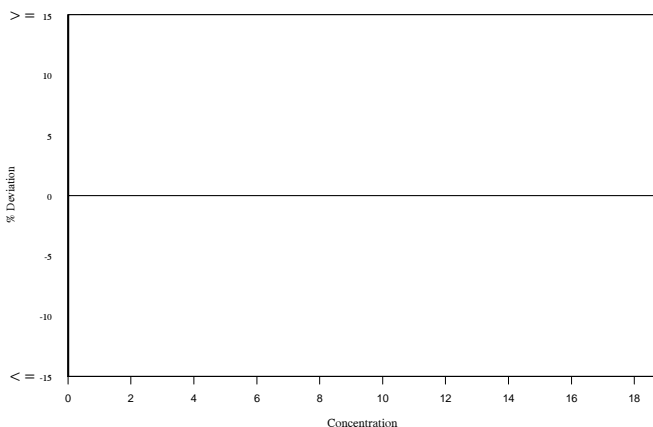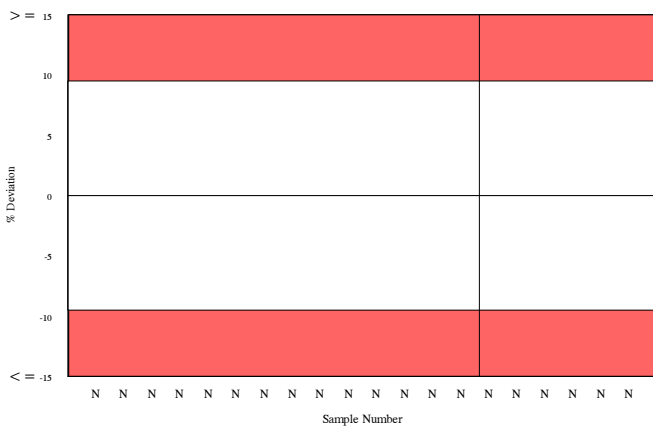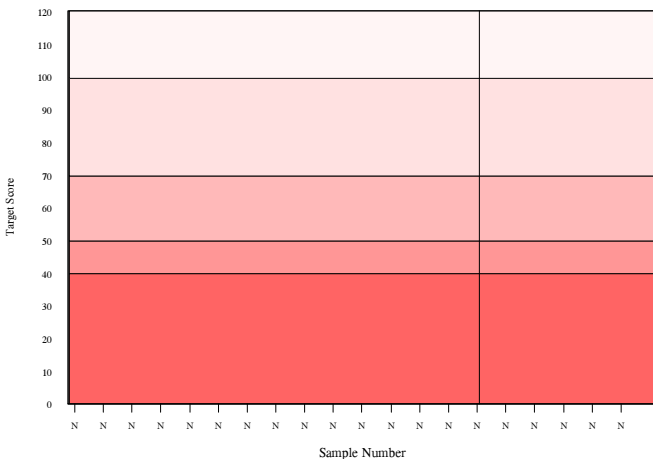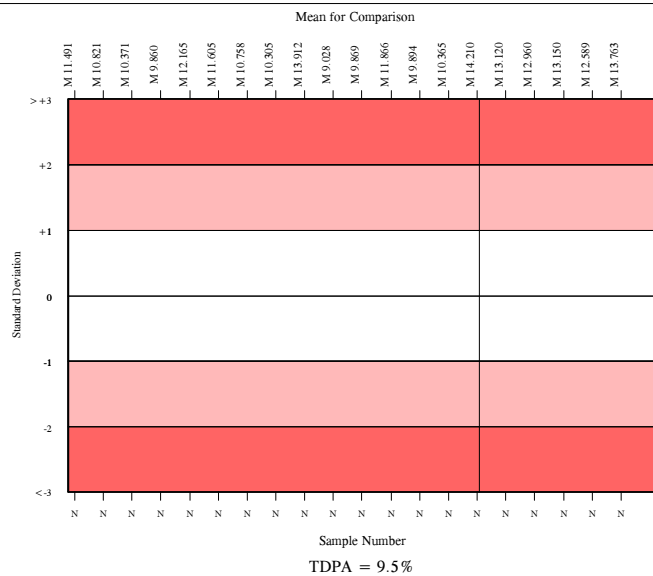


WBC (Impedance Count), x10³/mm³





	N	Mean	CV%	U _m	SDPA	Exc.
All Methods	2575	11.808	4.4	0.01	0.58	203
ABX Micros/Minos/ABC VET	156	11.393	4.4	0.05	0.56	15

▲ Your Result	10.800	SDI	-1.06
		RMSDI	Too Few
■ Mean for Comparison	11.393	TS	69
		RMTS	Too Few
		%DEV	-5.2
		RM%DEV	Too Few

Acceptable limits derived from Biological Variation	15.49%
Acceptable limits of performance for RIQAS	8.10%

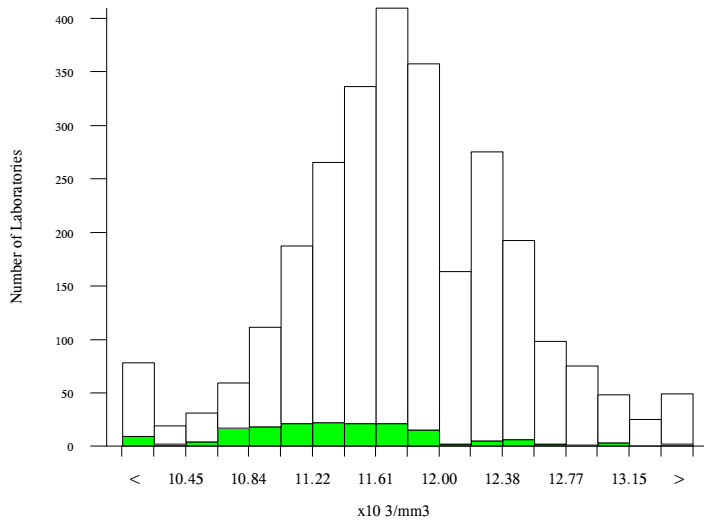

Method	N	Mean	CV%	U _m
Nihon Kohden Celltac F, Es, Alpha	254	11.430	2.9	0.03
Mindray BC 2000/3000 series	211	11.873	3.5	0.04
Sysmex KX 21	214	11.502	2.9	0.03
ABX Micros/Minos/ABC VET	156	11.393	4.4	0.05
Beckman Coulter LH700 Series	151	12.302	2.0	0.02
Beckman Coulter DxH Series	148	12.202	2.3	0.03
Sysmex XP Series	136	11.727	3.1	0.04
ABX Pentra	126	11.987	3.4	0.05
ABX Pentra 60/80 /Yumizen H500	96	11.808	3.1	0.05
Beckman Coulter Ac. T 5 series	97	11.989	2.1	0.03
Mindray BC 5100/5180/5300/5380	77	11.960	3.6	0.06
Medonic M series/Swelab	69	11.812	3.2	0.06
Abbott Cell-Dyn 3700	55	11.893	3.1	0.06
Abbott Cell-Dyn Emerald 18	45	11.594	3.7	0.08
Beckman Coulter HmX	44	12.493	3.2	0.08
Human Humacount Series	40	11.597	4.9	0.11
Abbott Cell-Dyn 1800	37	11.614	4.4	0.11
Beckman Coulter LH500 series	40	12.637	3.5	0.09
Abx Pentra 120/Nexus series	37	12.551	3.1	0.08
Sysmex XN-L Series (350/450/550)	29	11.974	2.1	0.06
Erba Lachema Elite series	26	11.821	5.0	0.14

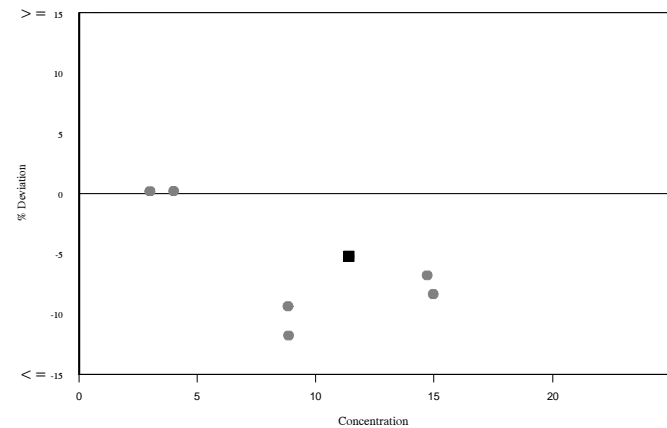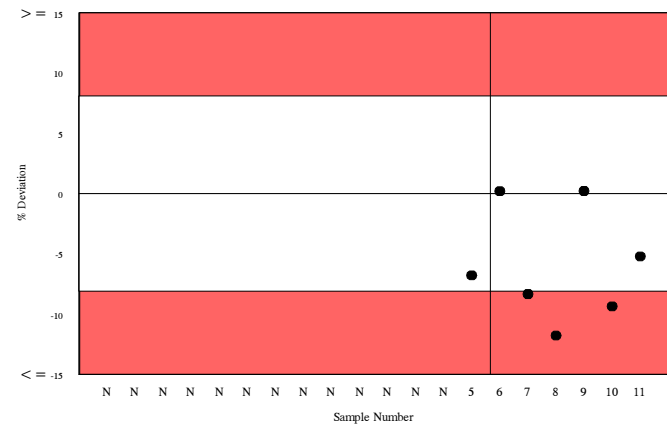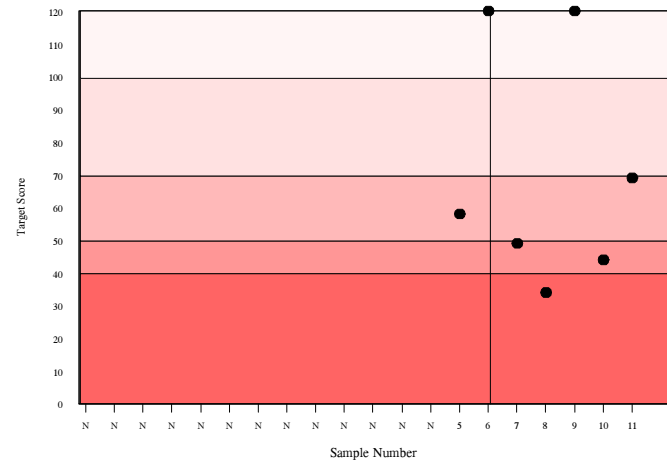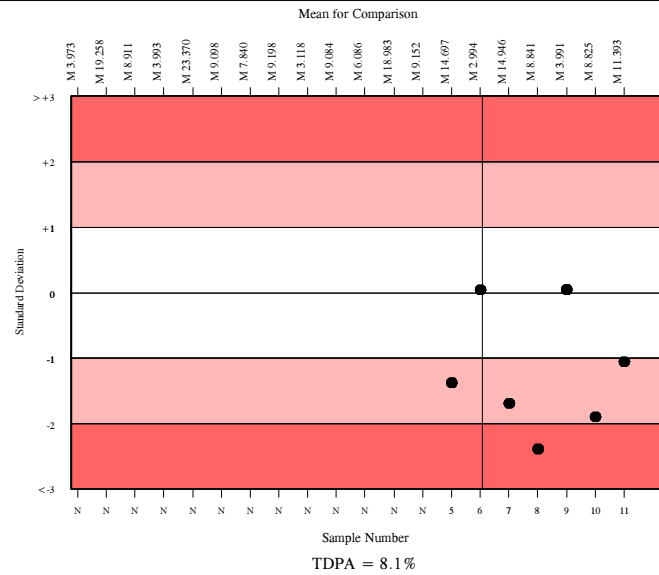

Analyte	Mean for Comparison	Your Result	SDI	RMSDI	%DEV	RM%DEV	TS	RMTS	Performance
Haemoglobin	14.292	14.700	1.09	Too Few	2.9	Too Few	68	Too Few	
Haematocrit (HCT)	42.908	43.900	0.62	Too Few	2.3	Too Few	92	Too Few	
MCH	28.453	28.600	0.17	Too Few	0.5	Too Few	120	Too Few	
MCHC	33.172	33.500	0.27	Too Few	1.0	Too Few	120	Too Few	
MCV	85.630	85.000	-0.24	Too Few	-0.7	Too Few	120	Too Few	
Mean Platelet Volume	8.749	8.600	-0.25	Too Few	-1.7	Too Few	120	Too Few	
Plateletcrit	0.219	No Result		Too Few		Too Few		Too Few	
Platelets (Impedance Count)	253.240	245.000	-0.42	Too Few	-3.3	Too Few	109	Too Few	
RBC (Impedance Count)	5.036	5.140	0.89	Too Few	2.1	Too Few	77	Too Few	
Red Cell Dist. Width CV	13.763	No Result		Too Few		Too Few		Too Few	
WBC (Impedance Count)	11.393	10.800	-1.06	Too Few	-5.2	Too Few	69	Too Few	

ORMSDI N/A

ORM%DEV N/A

ORMTS N/A

END OF REPORT

